



**S . M . T . L .**

subject: **Comparative Allewyn Wound Dressing Testing**

date: **24th March 2009**

from: **Victoria Baines  
Princess of Wales  
Tel: +44-1656-752820**

**Report No: 09/2896/1**

*Test Report*

09/2896/1

**1. Name & Address of Client/Requesting Authority.**

Ms Jessica Thompson  
Brand Manager (Allewyn)  
Smith and Nephew  
Healthcare House,  
Goulton Street  
Hull  
HU3 4DJ

Email: [jessica.thompson@smith-nephew.com](mailto:jessica.thompson@smith-nephew.com)

**2. Introduction**

The SMTL were requested by the client to perform comparative testing on Allewyn and Versiva XC foam wound dressings.

---

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

---

RCS Version Info: \$Header: /projects/2896/Reports/2896.report.v 1.11 2009/07/02 13:27:33 hugh Exp \$

09/2896/1

Page 1 of 13 Comparative Wound Dressing Testing

### 3. Test Product(s)/Sample(s)

**TABLE 1.** Test Product(s)/Sample(s) tested by SMTL.

Manufacturer	Item	Cat No	Batch/Lot No	Quantity	Date Received
Smith & Nephew	Allevyn Adhesive 10 x 10 cm	66000599	520318	40	19/12/2008
Smith & Nephew	Allevyn Adhesive 10 x 10 cm	66000599	520387	20	19/12/2008
Smith & Nephew	Allevyn Non-Adhesive 10 x 10cm	66157637	0839	30	19/12/2008
Smith & Nephew	Allevyn Non-Adhesive 10 x 10cm	66157637	0846	2	19/12/2008
ConvaTec	Versiva XC Adhesive 10 x 10cm	410609	3015639	30	19/12/2008
ConvaTec	Versiva XC Adhesive 10 x 10cm	410609	2807992	1	19/12/2008
ConvaTec	Versiva XC Non-Adhesive 11 x 11cm	410607	7F30046	30	19/12/2008
ConvaTec	Versiva XC Non-Adhesive 11 x 11cm	410607	7D28335	2	19/12/2008

**NOTE: The test results in this report relate only to the test sample(s) analysed.**

#### 3.1 Departures/Abnormalities of Sample Condition

None

### 4. Date of Testing

December 2008 - February 2009

### 5. Testing Details

#### 5.1 Moisture vapour permeability

The moisture vapour permeability of the dressings was determined using SMTL test method TM-8.<sup>(1)</sup>

In this test, a sample of dressing is applied to a Paddington cup to which is added 20 ml of a solution of sodium and calcium chloride containing 142 mmoles/litre of sodium ions and 2.5 mmoles/litre of calcium ions.

The cup is placed in an inverted position (with the test solution in contact with the sample) upon the pan of a top loading balance located within an incubator set at 37±2°C . The balance is connected to an electronic data logging device which records changes in the weight of the cup resulting from the loss of moisture vapour through the dressing. A tray containing 1 kg of freshly dried silica gel is placed in the bottom of the incubator to maintain a low relative humidity within the chamber.

At the end of the test the recorded data is down-loaded for examination.

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

## 5.2 Fluid handling properties

The fluid handling properties of the dressings were examined using SMTL test method TM-390,<sup>(2)</sup> which is written in accordance with the European Standard *BS EN 13726:1:2002 - Test methods for primary wound dressings. Part 1; Aspects of absorbency. Section 3.3 - Fluid Handling Capacity (absorbency plus moisture vapour transmission rate, liquid in contact)*.<sup>(3)</sup>

In this test, five samples of each dressing are applied to Paddington cups, to which are added 20 ml of a solution of sodium/calcium chloride containing 142 mmol/litre of sodium ions and 2.5 mmol/litre of calcium ions. The cups are weighed using a calibrated analytical balance and placed in a temperature and humidity controlled incubator used to maintain an environment of  $37\pm 2^{\circ}\text{C}$  and a relative humidity level below 20% for a period of 24 hours.

At the end of the test the cups are removed from the incubator, and are allowed to equilibrate at room temperature for a period of 30 minutes prior to reweighing on the analytical balance.

From these weighings the loss in weight due to the passage of moisture vapour through the dressing is determined. The base of each cup is then removed and any remaining fluid allowed to drain.† After a period of  $15\pm 2$  min the cup is then reweighed once again and the weight of fluid retained by the dressing calculated by difference.

This test can be repeated over a period of 48 hours.

## 5.3 Foam Absorbency Testing to BP Requirements

The absorbency of the dressings is determined using SMTL test method TM-366<sup>(4)</sup> which is written in accordance with the *British Pharmacopoeia 1993 Volume II, Polyurethane Foam Dressings*.<sup>(5)</sup>

Five dressing were sectioned into 5cm x 5cm samples. The weight of the samples were then determined using a calibrated balance. Dressings were then immersed in de-ionised water for 60 minutes, before being drained on a draining board inclined at  $45^{\circ}$  for 5 minutes. The weight of the samples after draining was then determined, and the individual increase in weight per sample calculated. The increase in weight shall be greater or equal to 7.5 times the dry weight.

---

† If there is an accumulation of test fluid between two components of the dressing, the inner component must be slit with a scalpel blade to allow free drainage of the entrapped fluid.

#### **5.4 Standards relevant to the test method.**

- *BS EN 13726-1:2002: Test methods for primary wound dressings. Aspects of absorbency. Section 3.3 Fluid handling capacity (plus moisture vapour transmission rate, liquid in contact)*<sup>(3)</sup>
- *British Pharmacopoeia 1993 Volume II, Polyurethane foam dressings*<sup>(5)</sup>

#### **5.5 Deviations/exclusions from, and additions to standard methods.**

The following deviations from the SMTL test method TM-390<sup>(2)</sup> were employed

- Tests were also performed over a 72 hour duration.
- 30ml of Solution A was added to the Paddington cups for all tests.

The following deviation from the SMTL test method TM-8<sup>(1)</sup> was employed

- 30ml of Solution A was added to the Paddington cups for all tests.

#### **5.6 Sampling Details**

All samples were selected and supplied by the client.

#### **5.7 Sample Preparation**

As stated in the SMTL test method.

---

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

---

## 6. Results


### 6.1 Moisture Vapour Transmission Rate

Results from MVTR experiments are presented in Tables 2 to 5. Data is also expressed graphically in Figures 1 to 4.

**TABLE 2.** Allevyn Adhesive Moisture Vapour Transmission Rate over 24 hours

	MVTR (g/m <sup>2</sup> /24Hrs)
<b>Run 1</b>	7737
<b>Run 2</b>	6595
<b>Run 3</b>	7584
<b>Mean</b>	7305

**Figure 1.** Allevyn Adhesive - Moisture Vapour Transmission

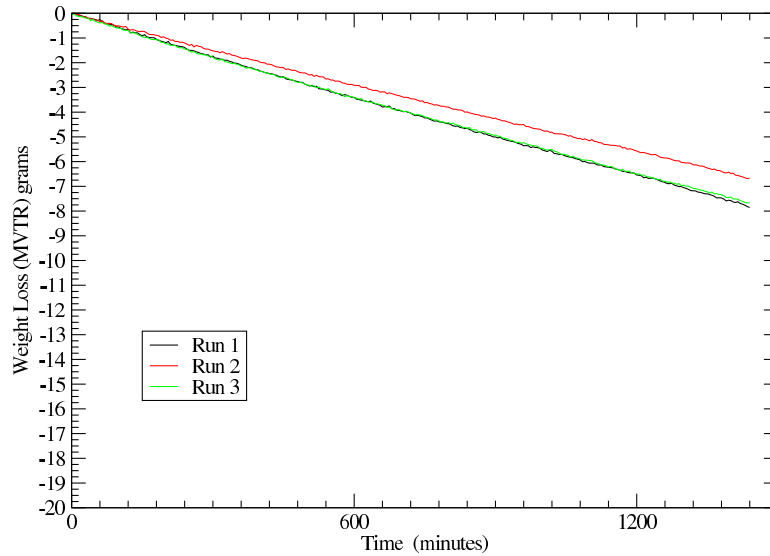


The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Colty Road, Bridgend, CF31 1RQ.

RCS Version Info: \$Header: /projects/2896/Reports/2896.report.v 1.11 2009/07/02 13:27:33 hugh Exp \$

**TABLE 3.** Versiva XC Adhesive Moisture Vapour Transmission Rate over 24 hours

	MVTR (g/m <sup>2</sup> /24Hrs)
<b>Run 1</b>	1086
<b>Run 2</b>	814
<b>Run 3</b>	1262
<b>Mean</b>	1054

**Figure 2.** Versiva XC Adhesive - Moisture Vapour Transmission

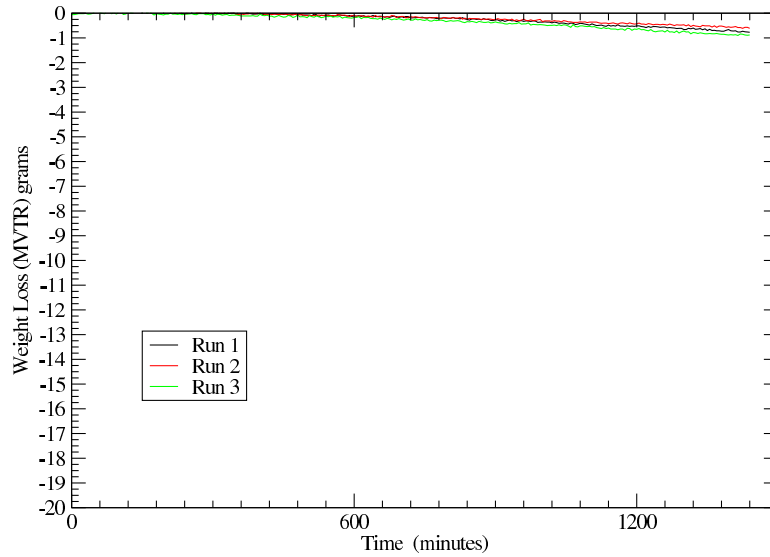


The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

**TABLE 4.** Alleevyn Non-Adhesive Moisture Vapour Transmission Rate over 24 hours

	MVTR (g/m <sup>2</sup> /24Hrs)
<b>Run 1</b>	11,645
<b>Run 2</b>	17,228
<b>Run 3</b>	18,880
<b>Mean</b>	15,917

**Figure 3.** Alleevyn Non-Adhesive - Moisture Vapour Transmission

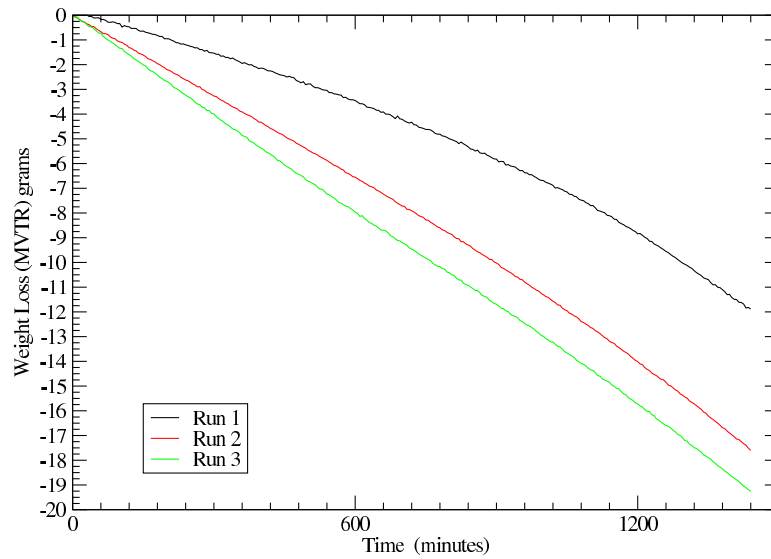


The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

**TABLE 5.** Versiva XC Non-Adhesive Moisture Vapour Transmission Rate over 24 hours

	MVTR (g/m <sup>2</sup> /24Hrs)
<b>Run 1</b>	1164
<b>Run 2</b>	1209
<b>Run 3</b>	1168
<b>Mean</b>	1180

**Figure 4.** Versiva XC Non-Adhesive - Moisture Vapour Transmission

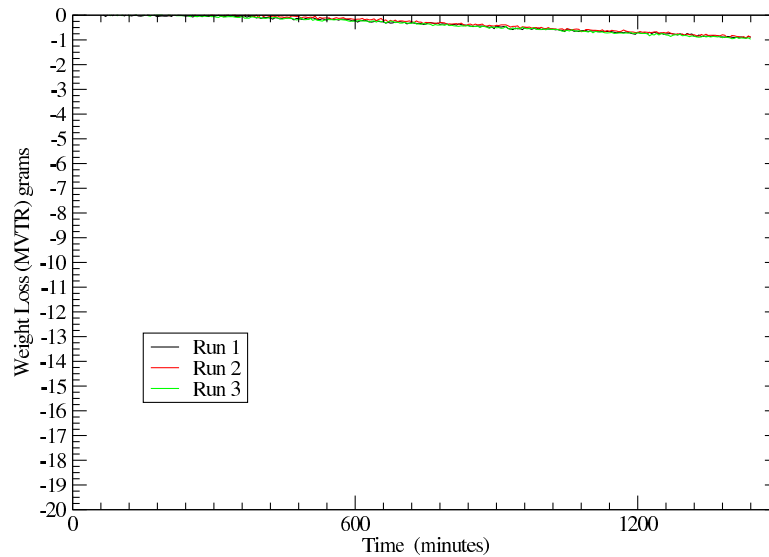

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

RCS Version Info: \$Header: /projects/2896/Reports/2896.report.v 1.11 2009/07/02 13:27:33 hugh Exp \$

## 6.2 Fluid Handling Testing

The results of the fluid handling testing are presented in Tables 6 to 8.

**TABLE 6.** Fluid handling properties following 24 hours incubation

Dressing	Moisture Vapour Loss (g/10cm <sup>2</sup> )	Absorbency (g/10cm <sup>2</sup> )	Fluid Handling Capacity (g/10cm <sup>2</sup> )
<b>Allevyn Adhesive</b>	10.957 (1.7401)	4.9599 (0.2179)	15.9172 (1.8875)
<b>Versiva XC Adhesive</b>	0.6871 (0.0928)	5.0375 (0.1331)	5.7246 (0.1930)
<b>Allevyn Non-Adhesive</b>	12.7836 (1.7718)	5.9149 (1.3370)	18.6985 (3.0764)
<b>Versiva XC Non-Adhesive</b>	0.8211 (0.0359)	5.1177 (0.0825)	5.9388 (0.1066)

**Note:**

- The results are the mean of 5 determinations
- Figures in brackets denote standard deviations

**TABLE 7.** Fluid handling properties following 48 hours incubation

Dressing	Moisture Vapour Loss (g/10cm <sup>2</sup> )	Absorbency (g/10cm <sup>2</sup> )	Fluid Handling Capacity (g/10cm <sup>2</sup> )
<b>Allevyn Adhesive †</b>	26.1871 (0.9757)	3.6951 (0.8930)	29.8822 (0.1304)
<b>Versiva XC Adhesive</b>	1.9667 (0.1533)	5.0997 (0.1629)	7.0664 (0.2637)
<b>Allevyn Non-Adhesive †</b>	27.8151 (1.5081)	2.1292 (1.4073)	29.9443 (0.1053)
<b>Versiva XC Non-Adhesive</b>	2.0896 (0.0244)	5.2102 (0.1704)	7.2998 (0.1654)

**Note:**

- The results are the mean of 5 determinations
- Figures in brackets denote standard deviations

† Little fluid remained in the Allevyn Adhesive and Non-Adhesive Paddington cups at the end of the testing period. There was no evidence of leakage during the test period and the dressings appear to handle nearly all of the fluid during the test. These results are an indication of the amount of fluid applied and not necessarily the fluid handling capacity of the dressing.

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

**TABLE 8.** Fluid handling properties following 72 hours incubation

Dressing	Moisture Vapour Loss (g/10cm <sup>2</sup> )	Absorbency (g/10cm <sup>2</sup> )	Fluid Handling Capacity (g/10cm <sup>2</sup> )
<b>Allevyn Adhesive ‡</b>	-	-	-
<b>Versiva XC Adhesive</b>	3.1758 (0.1167)	5.3867 (0.1441)	8.56248 (0.1045)
<b>Allevyn Non-Adhesive ‡</b>	-	-	-
<b>Versiva XC Non-Adhesive</b>	3.1668 (0.0383)	5.3881 (0.1688)	8.5550 (0.1522)

**Note:**

- The results are the mean of 5 determinations
- Figures in brackets denote standard deviations

‡ As presented in the 48 hour test data (Table 7) the Allevyn Adhesive and Non-Adhesive dressings handle the maximum capacity of test fluid the Paddington cups can hold within 48 hours of incubation, and therefore the dressings were not subjected to the 72 hour testing.

### 6.3 BP Foam Absorbency

The results from the absorbency determination are presented in Tables 9 and 12.

**TABLE 9.** Absorbency of Allevyn Adhesive dressings

Sample No.	Sample weight (g)	Final Weight (g)	Weight increase Factor	Complies/ Does not comply †
1	1.30	14.54	10.18	Complies
2	1.28	15.44	11.06	Complies
3	1.39	14.69	9.57	Complies
4	1.42	15.55	9.95	Complies
5	1.47	16.97	10.54	Complies

**Note:**

† For compliance weight increase factor shall be greater or equal to 7.5.

**TABLE 10.** Absorbency of Versiva XC Adhesive dressings

Sample No.	Sample weight (g)	Final Weight (g)	Weight increase Factor	Complies/ Does not comply †
1	2.69	11.34	3.22	Does not comply
2	2.53	11.36	3.49	Does not comply
3	2.60	11.53	3.43	Does not comply
4	2.51	11.70	3.66	Does not comply
5	2.43	11.53	3.74	Does not comply

**Note:**

† For compliance weight increase factor shall be greater or equal to 7.5.

---

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

**TABLE 11.** Absorbency of Allewyn Non-Adhesive dressings

Sample No.	Sample weight (g)	Final Weight (g)	Weight increase Factor	Complies/ Does not comply †
1	1.64	22.20	12.54	Complies
2	1.79	23.89	12.35	Complies
3	1.71	21.87	11.79	Complies
4	1.64	22.31	12.60	Complies
5	1.60	23.81	13.88	Complies

**Note:**

† For compliance weight increase factor shall be greater or equal to 7.5.

**TABLE 12.** Absorbency of Versiva XC Non- Adhesive dressings

Sample No.	Sample weight (g)	Final Weight (g)	Weight increase Factor	Complies/ Does not comply †
1	2.57	12.02	3.68	Does not comply
2	2.52	13.04	4.17	Does not comply
3	2.52	12.75	4.06	Does not comply
4	2.56	13.34	4.21	Does not comply
5	2.59	13.17	4.08	Does not comply

**Note:**

† For compliance weight increase factor shall be greater or equal to 7.5.



Peter Phillips, Director, SMTL.

Date: 26th March 2009

---

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

---

*References*

1. Surgical Materials Testing Lab., "Moisture Vapour Transmission Rate from Dressings by Electronic Data Capture Method," TM-8 Q.
2. Surgical Materials Testing Lab., "Fluid Handling Capacity BS EN 13726-1:2002," TM-390 Q.
3. "Test methods for primary wound dressings. Part 1; Aspects of absorbency. Section 3.3 - Fluid Handling Capacity (absorbency plus moisture vapour transmission rate, liquid in contact)," *BS EN 13726-1 Section 3.3*, British Standards Institution, (2002).
4. Surgical Materials Testing Lab., , "Foam Absorbency Testing to BP Requirements," TM-366 Q.
5. "Surgical Dressings: Polyurethan Foam Dressings," *BP 1993 Volume II*, British Pharmacopoeia, (1993 Vol II).

---

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

---

RCS Version Info: \$Header: /projects/2896/Reports/2896.report.v 1.11 2009/07/02 13:27:33 hugh Exp \$

## CONTENTS

1. Name & Address of Client/Requesting Authority.....	1
2. Introduction .....	1
3. Test Product(s)/Sample(s).....	2
3.1 Departures/Abnormalities of Sample Condition.....	2
4. Date of Testing.....	2
5. Testing Details .....	2
5.1 Moisture vapour permeability.....	2
5.2 Fluid handling properties .....	3
5.3 Foam Absorbency Testing to BP Requirements.....	3
5.4 Standards relevant to the test method.....	4
5.5 Deviations/exclusions from, and additions to standard methods.....	4
5.6 Sampling Details.....	4
5.7 Sample Preparation .....	4
6. Results .....	5
6.1 Moisture Vapour Transmission Rate.....	5
6.2 Fluid Handling Testing.....	9
6.3 BP Foam Absorbency .....	11

---

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

---

RCS Version Info: \$Header: /projects/2896/Reports/2896.report.v 1.11 2009/07/02 13:27:33 hugh Exp \$

LIST OF FIGURES

Figure 1. Allevyn Adhesive - Moisture Vapour Transmission..... 5  
Figure 2. Versiva XC Adhesive - Moisture Vapour Transmission ..... 6  
Figure 3. Allevyn Non-Adhesive - Moisture Vapour Transmission ..... 7  
Figure 4. Versiva XC Non-Adhesive - Moisture Vapour Transmission ..... 8

---

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

---

RCS Version Info: \$Header: /projects/2896/Reports/2896.report.v 1.11 2009/07/02 13:27:33 hugh Exp \$

## LIST OF TABLES

TABLE 1. Test Product(s)/Sample(s) tested by SMTL.....	2
TABLE 2. Allewyn Adhesive Moisture Vapour Transmission Rate over 24 hours.....	5
TABLE 3. Versiva XC Adhesive Moisture Vapour Transmission Rate over 24 hours .....	6
TABLE 4. Allewyn Non-Adhesive Moisture Vapour Transmission Rate over 24 hours.....	7
TABLE 5. Versiva XC Non-Adhesive Moisture Vapour Transmission Rate over 24 hours.....	8
TABLE 6. Fluid handling properties following 24 hours incubation .....	9
TABLE 7. Fluid handling properties following 48 hours incubation .....	9
TABLE 8. Fluid handling properties following 72 hours incubation .....	10
TABLE 9. Absorbency of Allewyn Adhesive dressings.....	11
TABLE 10. Absorbency of Versiva XC Adhesive dressings .....	11
TABLE 11. Absorbency of Allewyn Non-Adhesive dressings .....	12
TABLE 12. Absorbency of Versiva XC Non- Adhesive dressings.....	12

---

The information contained in this report is proprietary, and is not for circulation without the consent of the Surgical Material Testing Laboratory (S. M. T. L.), or the commissioning authority/company. This report shall not be reproduced except in full without the written approval of S. M. T. L., Princess of Wales Hospital, Coity Road, Bridgend, CF31 1RQ.

---

RCS Version Info: \$Header: /projects/2896/Reports/2896.report.v 1.11 2009/07/02 13:27:33 hugh Exp \$

---

*The information contained herein is for the use of employees and clients of S. M. T. L. and is not for publication. The report shall not be reproduced except in full without the written approval of S. M. T. L. (see BS 7501:1989)*

---

Title: **Comparative Allevyn Wound Dressing Testing**

Date: **24th March 2009**

Other Keywords:

Report No: **09/2896/1**

Author(s)  
**Victoria Baines**

Location  
**Princess of Wales**

Extension

Charging\ Cas**09/2896/1**  
Filing\ Case:

---

Pages Text: 16	Other: 0	Total: 16
No. Figures: 4	No. Tables: 12	No. Refs.: 0

---